Singapore Test Services Pte Ltd
Block 4010 Techplace 1
Ang Mo Kio Ave 10 #03 ±8 to 12
Singapore 569626

Certificate No. : LA-1987-0012-C

Issue No. : 25

Date : 28 November 2017

FIELD OF TESTING : Calibration and Measurement

MEASURED QUANTITIES/ RANGE/ INSTRUMENTS TO BE CALIBRATED	METHOD	CALIBRATION & MEASUREMENT CAPABILITY EXPRESSED AS AN UNCERTAINTY (*)
A. MECHANICAL **A.I. Pressure**		

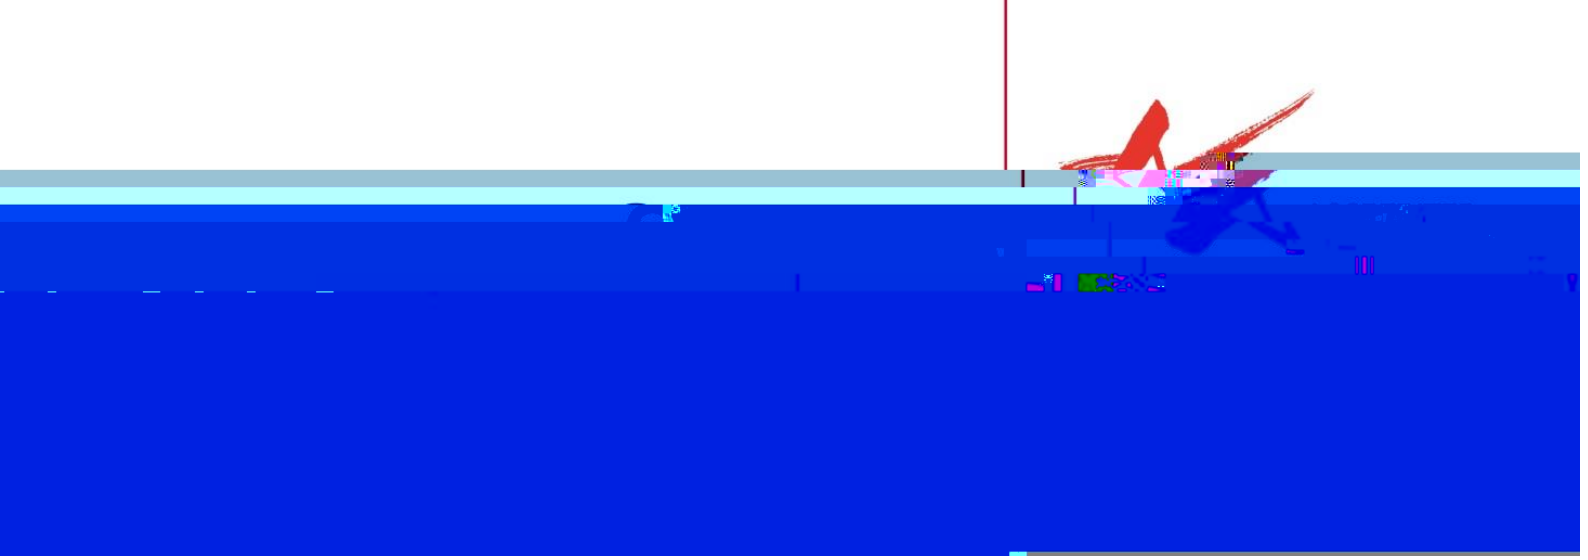

MEASURED QUANTITIES/ RANGE/ INSTRUMENTS TO BE CALIBRATED	METHOD	CALIBRATION & MEASUREMENT CAPABILITY EXPRESSED AS AN UNCERTAINTY (*)
A.II FORCE MEASUREMENT		
10 Calibration of Durometer (Verification of the test force)		
a. ASTM D 2240:2015 Type A	STS in-house procedure T-WI-CMD-003-19 Rev 10	0.0080 N

Certificate No. : LA-1987-0012-C Issue No. : 25

Date : 28 Novemf598 rtificate

MEASURED QUANTITIES/ RANGE/ INSTRUMENTS TO BE CALIBRATED	METHOD	CALIBRATION & MEASUREMENT CAPABILITY EXPRESSED AS AN UNCERTAINTY (*)
8b Temperature Simulator (Source)	STS in-house procedure T-WI-CMD	

MEASURED QUANTITIES/
RANGE/ INSTRUMENTS

MEASURED QUANTITIES/ RANGE/ INSTRUMENTS TO BE CALIBRATED	METHOD	CALIBRATION & MEASUREMENT CAPABILITY EXPRESSED AS AN UNCERTAINTY (*)
D. ELECTRICAL		

MEASURED QUANTITIES/ RANGE/ INSTRUMENTS TO BE CALIBRATED	METHOD	CALIBRATION & MEASUREMENT CAPABILITY EXPRESSED AS AN UNCERTAINTY0 1 27

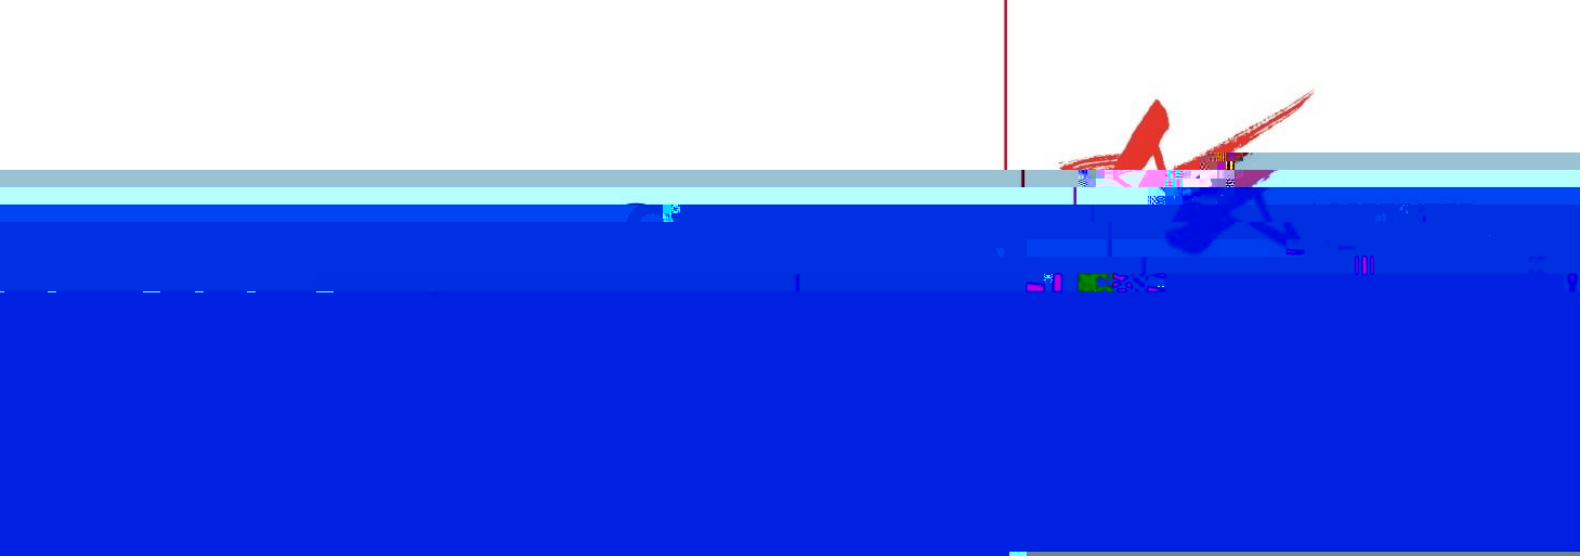

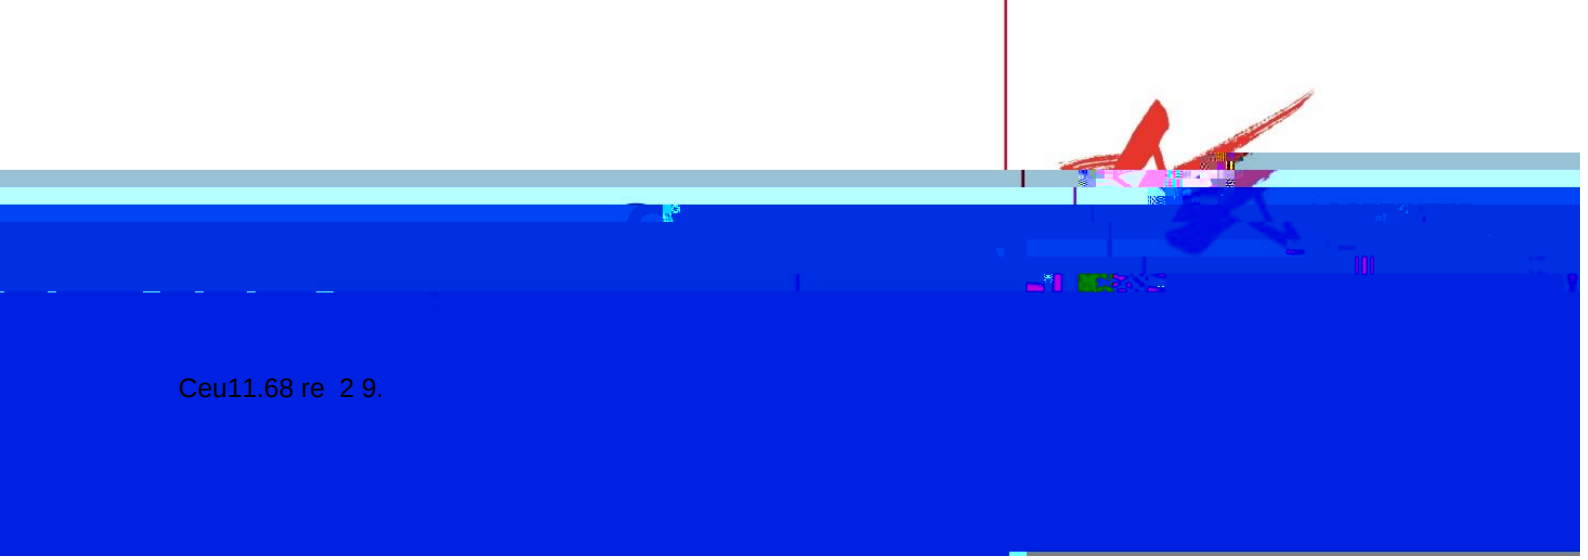

Ceu11.68 re 2 9.

Approved signatories

Name	Cat. A Mechanical	Cat. B Dimensional	Cat. C Temperature	Cat. D Electrical	Cat. E Optical
Mr Mohd Haron B. Junaidi	A(I), Ao7 Tm 0 g 0 G				